

Comparative Evaluation of Dentinal Defects Caused by Different Rotary Ni-ti Instruments: A In Vitro Study

Dr. Smita Sahni¹, Dr. Anil K. Tomer², Dr. Shobhit Kumar Pyasi³

PG Student^{1,3}, Professor & HOD², Department of Conservative & Endodontics, DJ College of Dental Science, Modinagar, Ghaziabad

Abstract:

Aim: This study was carried out to compare the dentinal defects induced by three different rotary file system 2 shape (Micro-Mega, Besancon, Cedex, France), Neolix (Neolix, châtres-la-Forêt, France) and Protaper universal (Dentsply Maillefer, Ballaigues, Switzerland).

Materials & Methods: Eighty single-rooted mandibular premolars were selected based on predetermined criteria. Twenty teeth were left unprepared and served as a negative control (Group I). The remaining sixty teeth was divided into three groups: Group II (Pro taper universal), group III (neolix) and group IV (2 Shape). Biomechanical preparation was carried out as per the manufacturer's instructions. After root canal preparation, all of the roots were sectioned perpendicular to the long axis at 3, 6, and 9 mm from the apex. These sections were visualized under stereo microscope to evaluate the dentinal defects using predetermined criteria. The absence/presence of cracks was recorded, and the data were analyzed with a chi-square test. The significance level was set at $P=0.05$.

Results: Roots prepared with ProTaper Universal showed maximum defects, whereas no significant difference was found in dentinal defects in roots prepared with neolix and 2 shape files. There was statistically significant difference between the Protaper group and other two groups ($p < 0.05$).

Conclusion: All of the NiTi files tested in the present study were found to cause dentinal defect. Statistical analysis showed no significant difference in root dentinal crack formation between 2 shape and Neolix rotary systems.

How to cite this Article: Sahni S, Tomer AK, Pyasi S. Comparative Evaluation of Dentinal Defects Caused by Different Rotary Ni-ti Instruments: A In Vitro Study. HTAJOCD.2018;11(2):51-52

Introduction

A successful endodontic therapy is based upon triad of proper diagnosis, thorough biomechanical preparation and three dimensional obturation of root canal system. The chemo-mechanical root canal preparation involves preservation of the original course of the canal and removal of bacteria from the entire root canal system¹.

With recent advances in dental technology, various nickel-titanium instruments with different designs have been introduced. A common complication of mechanical canal preparation is vertical root fracture (VRF)². It has not yet been determined, whether even minor dentinal defects could lead to root fractures; therefore, steps should be taken to prevent occurrence of such defects

However, several factors like force of instrumentation and obturation; retreatment procedure and high concentration of hypochlorite may also be responsible for the formation of dentinal defects in different degrees. A weakened root, as a result of flaring and instrumentation, could suffer VRFs during obturation procedures⁴.

The purpose of this study is to compare the damage observed in root dentin after endodontic preparations with different Ni-Ti rotary file systems.

Material and Methods

Eighty extracted mandibular premolars were selected and cleaned with periodontal scaler and stored in purified filtered water. The coronal portions of all teeth were removed with diamond disk, leaving roots 16 mm in length. All root surfaces were observed with stereo microscope under $\times 12$ to exclude cracks.

Patency of the canal was established using #10 K-File (Mani, Japan) in the canal.

The cemental surface of the root was coated with light body impression material and embedded into the acrylic blocks to simulate the periodontal ligament and avoid the external reinforcement. The specimens were then

divided into four groups; each group containing 20 specimens each.

Group I: Left unprepared and served as Group I.

Group II: Twenty specimens were prepared using Endo Motor (X Smart Dentsply) and Protaper universal rotary files (Dentsply) using crown down technique according to the manufacturer's instructions.

Group III: Thirty specimens were prepared with Endo Motor (X Smart Dentsply) and Neolix (Neolix, châtres-la-Forêt, France) using crown down technique according to the manufacturer's instructions

Group IV: Thirty specimens were prepared with Endo Motor (X Smart Dentsply) and 2 Shape Single file rotary system (Micro Mega) using crown down technique according to the manufacturer's instructions.

In all the groups, canals were irrigated with 2.5% sodium hypochlorite (NaOCl) solution between each instrument and Glyde EDTA Gel (17%) was used during the preparation procedure. All roots were kept moist through out the experimental procedures to prevent dehydration.

Sectioning and Microscopic Observations

All roots were cut horizontally at 3, 6, and 9 mm from the apex. Sections were then viewed under stereo microscope. The appearance of dentinal defects was registered by the pictures that were taken digitally.

Roots were classified as "defected" if at least one of the three sections showed either a craze line, partial crack or a fracture. Results were expressed as the number and percentage of defected roots in each group.

The defects observed were scored and classified under following predetermined criteria:

- "No defect" was observed as root dentine devoid of any lines or cracks where both the external surface of the root and the internal root canal wall had no defects.
- "Fracture" was observed as a line extending from the root canal space to the outer surface

of the root.

- "Craze line" line extending from the outer surface into the dentine that did not reach the canal lumen
- "Partial crack" line extending from the canal wall into the dentine without reaching the outer surface of the root.

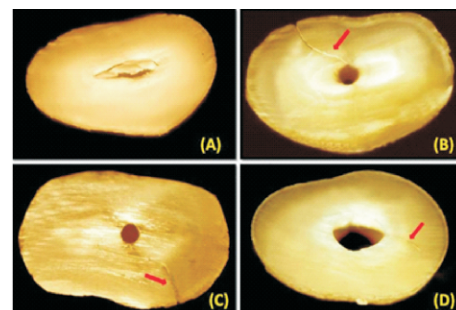


Fig -1 Various Dentinal Defects

Statistical Analysis

The data were analyzed using statistical software program. A Chi-square test was performed to determine statistically significant difference in the appearance of defected roots between the experimental groups. Chi-square test was also performed to determine the defects at different horizontal sections in each group. The level of significance was set at $P < 0.05$.

Results

Figure 2 is a bar chart representing the number of root defects in each group.

The teeth in the control group showed no defects. The maximum percentage of defect was seen in the teeth instrumented using Protaper universal file system (8/20) (40%). The percentage of defects seen in the other two groups are neolix (2/20) (10%), and 2 shape (1/20) (5%). Statistical significant difference was seen between protaper universal and the other two rotary groups. No significant difference was found between the neolix and 2 shape group ($P > 0.05$). All experimental groups demonstrated significantly more defects at the 3 mm level when compared with the unprepared group.



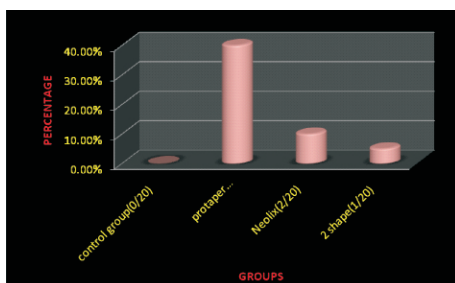


Fig-2 Bar Chart
Representing Percentage of Root Defects

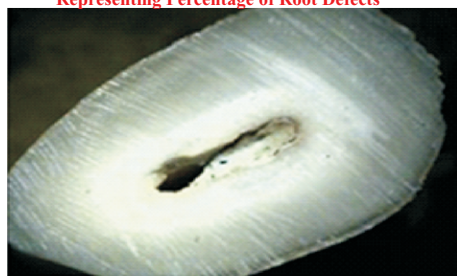

Group II (protaper universal)

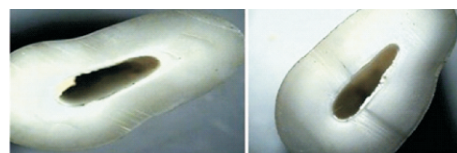

Group III (Neolix) Group IV (2 shape)

Fig-3 Stereo microscopic
Images Showing Dentinal Defects

Discussion

Many new NiTi rotary instruments have been developed and introduced by various manufacturers. Majority of practitioners prefer these systems because of their advantages such as saving time and better cutting efficiency. Root canal preparation with larger tapered rotary NiTi instruments involves more dentin removal, which compromises the fracture strength of the roots leading to vertical root fracture⁵.

During the bio mechanical preparation, rotational forces applied on the walls of the root canal result in formation of microcracks or craze lines⁶. While using rotary files formation of these defects can be caused by many factors. Tip design, cross section geometry, constant or variable taper, and pitch and flute form⁷. In the present study, dentinal defects occurred in around 10% of total number of samples tested and in 40% of the sample in the protaper group, and these may develop into fractures following any additional procedure such as preparation, obturation, and retreatment or by repeated stress of occlusal forces. Bier et al. reported that craze lines occurred in 4 to 16% samples⁸. On ninket al. were the first to report dentinal defects as a consequence of canal preparation but only found small defects entirely within dentin that did not communicate with the canal wall⁹.

Sectioning method using diamond disk used in the present study could also result in dentinal defects. However, because both the control group did not show any defect, we may conclude that the defects seen were not due to sectioning procedure used.

Mandibular premolars were selected for the study because of the high prevalence of VRF as reported by Tamseet al¹⁰. It was also reported that occlusal load on mandibular premolars during chewing is three times as high as the other teeth.

The amount of material removed from the root canal depends on the shape of the rotary instrument and the penetration depth in the canal¹¹. Further more, the higher number of rotations in the canal necessary to complete a preparation with rotary Ni-Ti files with large taper, may contribute to the formation of dentinal defects.

File design, however, is also likely to affect the shaping forces on the root dentin. Forces generated during instrumentation have been linked to an increased risk of root fracture¹². During preparation, a canal is shaped by the contact between instrument and dentin walls. These contacts create many momentary stress concentrations in dentin. Such stress concentrations may leave dentinal defects in which VRF can initiate¹³. Higher stresses in the root during instrumentation can be expected to increase dentinal defects and thus increase VRF risk¹⁴.

ProTaper had 40% of dentinal defects as compared to other rotary systems which was significantly different. ProTaper rotary files are with progressive taper design which increases stiffness and facilitates active cutting motion and removes relatively more dentin coronally compared with other systems. ProTaper file F2 has a large taper of 0.08 which could explain the higher incidence of damage than other tapered rotary files. Bier et al. observed cracks in the horizontal sections of 16% of the roots instrumented with the ProTaper system and reported that ProTaper rotary files created more dentin damage than other rotary instruments¹⁵.

Neolix (Neolix, châtres-la-Forêt, France) and 2 shape both groups showed presence of dentinal defects in form of partial or complete cracks. Neolix has a non-homothetic rectangular section along the blade enabling a progressive flexibility to better negotiate the curves and respect the canal anatomy. It is a single file system which has an inbuilt abrasive property of the flutes and edges associate a grater and cutting action, avoiding smear layer risk. Its ability to conform to the root anatomy and greater flexibility may be the reason for less number of dentinal defects seen in his group.

2 shape file system produced the least number of defects. It has a triple helix cross-section with two main cutting edges and one secondary cutting edge for debris removal. The asymmetrical cross section allows for increased efficacy of the circumferential brushing movements for efficient selective cleaning thus reducing the incidence of dentinal defects created during cleaning and shaping of root canal¹⁶.

In the present study, a uniform tapered preparation (0.06-0.08) was attempted in all groups. The observation that all groups prepared showed various degrees of damage supports the idea that greater tapered files may generate an

increased stress on the dentin wall. Fewer microcrack formations occurred in apical thirds than middle and coronal thirds. In 2013, Liu et al. reported that during the instrumentation procedure, the stresses generated at 1 mm short of the Apical Foramen were merely one-third of the stress at more coronal levels¹⁷.

Conclusion

With in the limitation of the study it can be concluded that all the rotary instruments, induce dentinal defects, with protaper universal producing a higher number of defects as compared to the other two groups. Reasons may be the greater taper, more rotations and aggressive cutting which can generate increased stresses on the dentin wall and subsequent formation of dentinal defects.

Conflicts of interest.

There are no conflicts of interest.

References

- Peters OA. Current challenges and concepts in the preparation of root canal systems: A review. J Endod 2004;30:559-67.
- Bier CA, Shemesh H, Tanomaru-Filho M, Wesselink PR, Wu MK. The ability of different nickel-titanium rotary instruments to induce dentinal damage during canal preparation. J Endod 2009;35:236-8.
- Singh S, Nigam N. Comparative evaluation of surface characteristics of dentinal walls with and without using plastic finishing file. J Conserv Dent 2010;13:89-93.
- Kim HC, Lee MH, Yum J, Versluis A, Lee CJ, Kim BM. Potential relationship between design of nickel-titanium rotary instruments and vertical root fracture. J Endod 2010;36:1195-9.
- Pasqualini D, Scotti N, Tamagnone L, Ellena F, Berutti E. Hand-operated and rotary ProTaper instruments: A comparison of working time and number of rotations in simulated root canals. J Endod 2008;34:314-7.
- Shemesh H, Bier CA, Wu MK, Tanomaru-Filho M, Wesselink PR. The effects of canal preparation and filling on the incidence of dentinal defects. Int Endod J 2009;42:208-13.
- Barreto MS, Moraes Rdo A, Rosa RA, Moreira CH, Sô MV, Bier CA. Vertical root fractures and dentin defects: Effects of root canal preparation, filling, and mechanical cycling. J Endod 2012;38:1135-9.
- Onnink PA, Davis RD, Wayman BE. An in vitro comparison of incomplete root fractures associated with three obturation techniques. J Endod 1994;20:32-7.
- Shemesh H, Roeleveld AC, Wesselink PR, Wu MK. Damage to root dentin during retreatment procedures. J Endod 2011;37:63-6.
- Yoldas O, Yilmaz S, Atakan G, Kuden C, Kasan Z. Dentinal microcrack formation during root canal preparations by different NiTi rotary instruments and the self-adjusting file. J Endod 2012;38:232-5.
- Adorno CG, Yoshioka T, Suda H. The effect of root preparation technique and instrumentation length on the development of apical root cracks. J Endod 2009;35:389-92.
- Ruddle CJ. Endodontic disinfection tsunami irrigation. Endod Prac 2008;11:7-15.
- Slutzky-Goldberg I, Marec M, Liberman R, Heling I. Effect of sodium hypochlorite on dentin micro hardness. J Endod 2004;30:880-2.
- Yoldas O, Yilmaz S, Atakan G, Kuden C, Kasan Z. Dentinal microcrack formation during root canal preparations by different NiTi rotary instruments and the self-adjusting file. J Endod 2012;38:232-5.
- Hin ES, Wu MK, Wesselink PR, Shemesh H. Effects of self-adjusting file, Mtwo, and ProTaper on the root canal wall. J Endod 2013;39:262-4.
- Sathorn C, Palamara JE, Palamara D, Messer HH. Effect of root canal size and external root surface morphology on fracture susceptibility and pattern: A finite element analysis. J Endod 2005;31:288-92.
- Liu R, Hou BX, Wesselink PR, Wu MK, Shemesh H. The incidence of root microcracks caused by 3 different single file systems versus the ProTaper system. J Endod 2013;39:1054-6.